

Surgical protocol for



- optimized, bone quality-oriented set of instruments and surgical protocol for unsurpassed primary stability
- Drills with detachable drill stops
- Reduction of the number of drills for increased control and dependability during surgery


Implant length




Crestal drill




Hard bone D1

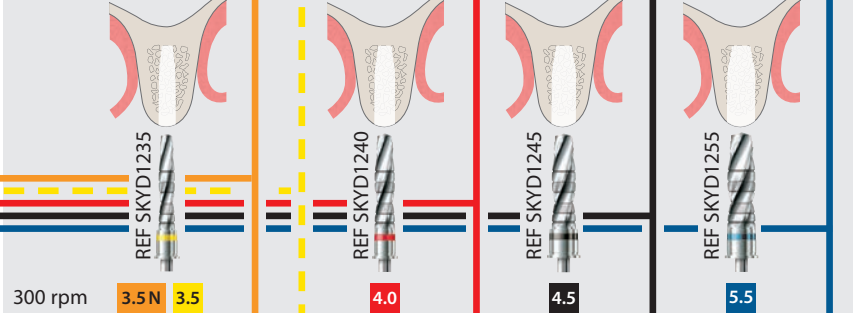

Medium hard / soft bone D2-D4

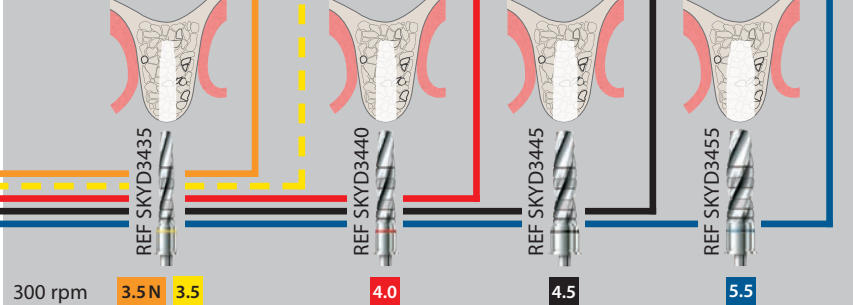


Pilot drill



800 - 1.000 rpm

Twistdrill




With the 3.5 diameter blueSKY and SKY classic implants, the crestal drill is only sunk up to the laser marking.

In the following implants:

- narrowSKY
- blueSKY 4.0 to 5.5
- SKY classic 4.0 to 4.5

the crestal drill is completely inserted.

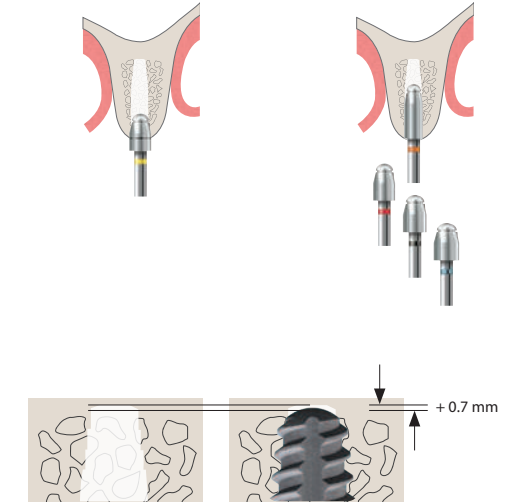

Detachable drill stops

